


LPT: Pompano Flow Test. Sample Interval Is 5 Mins

Pressure

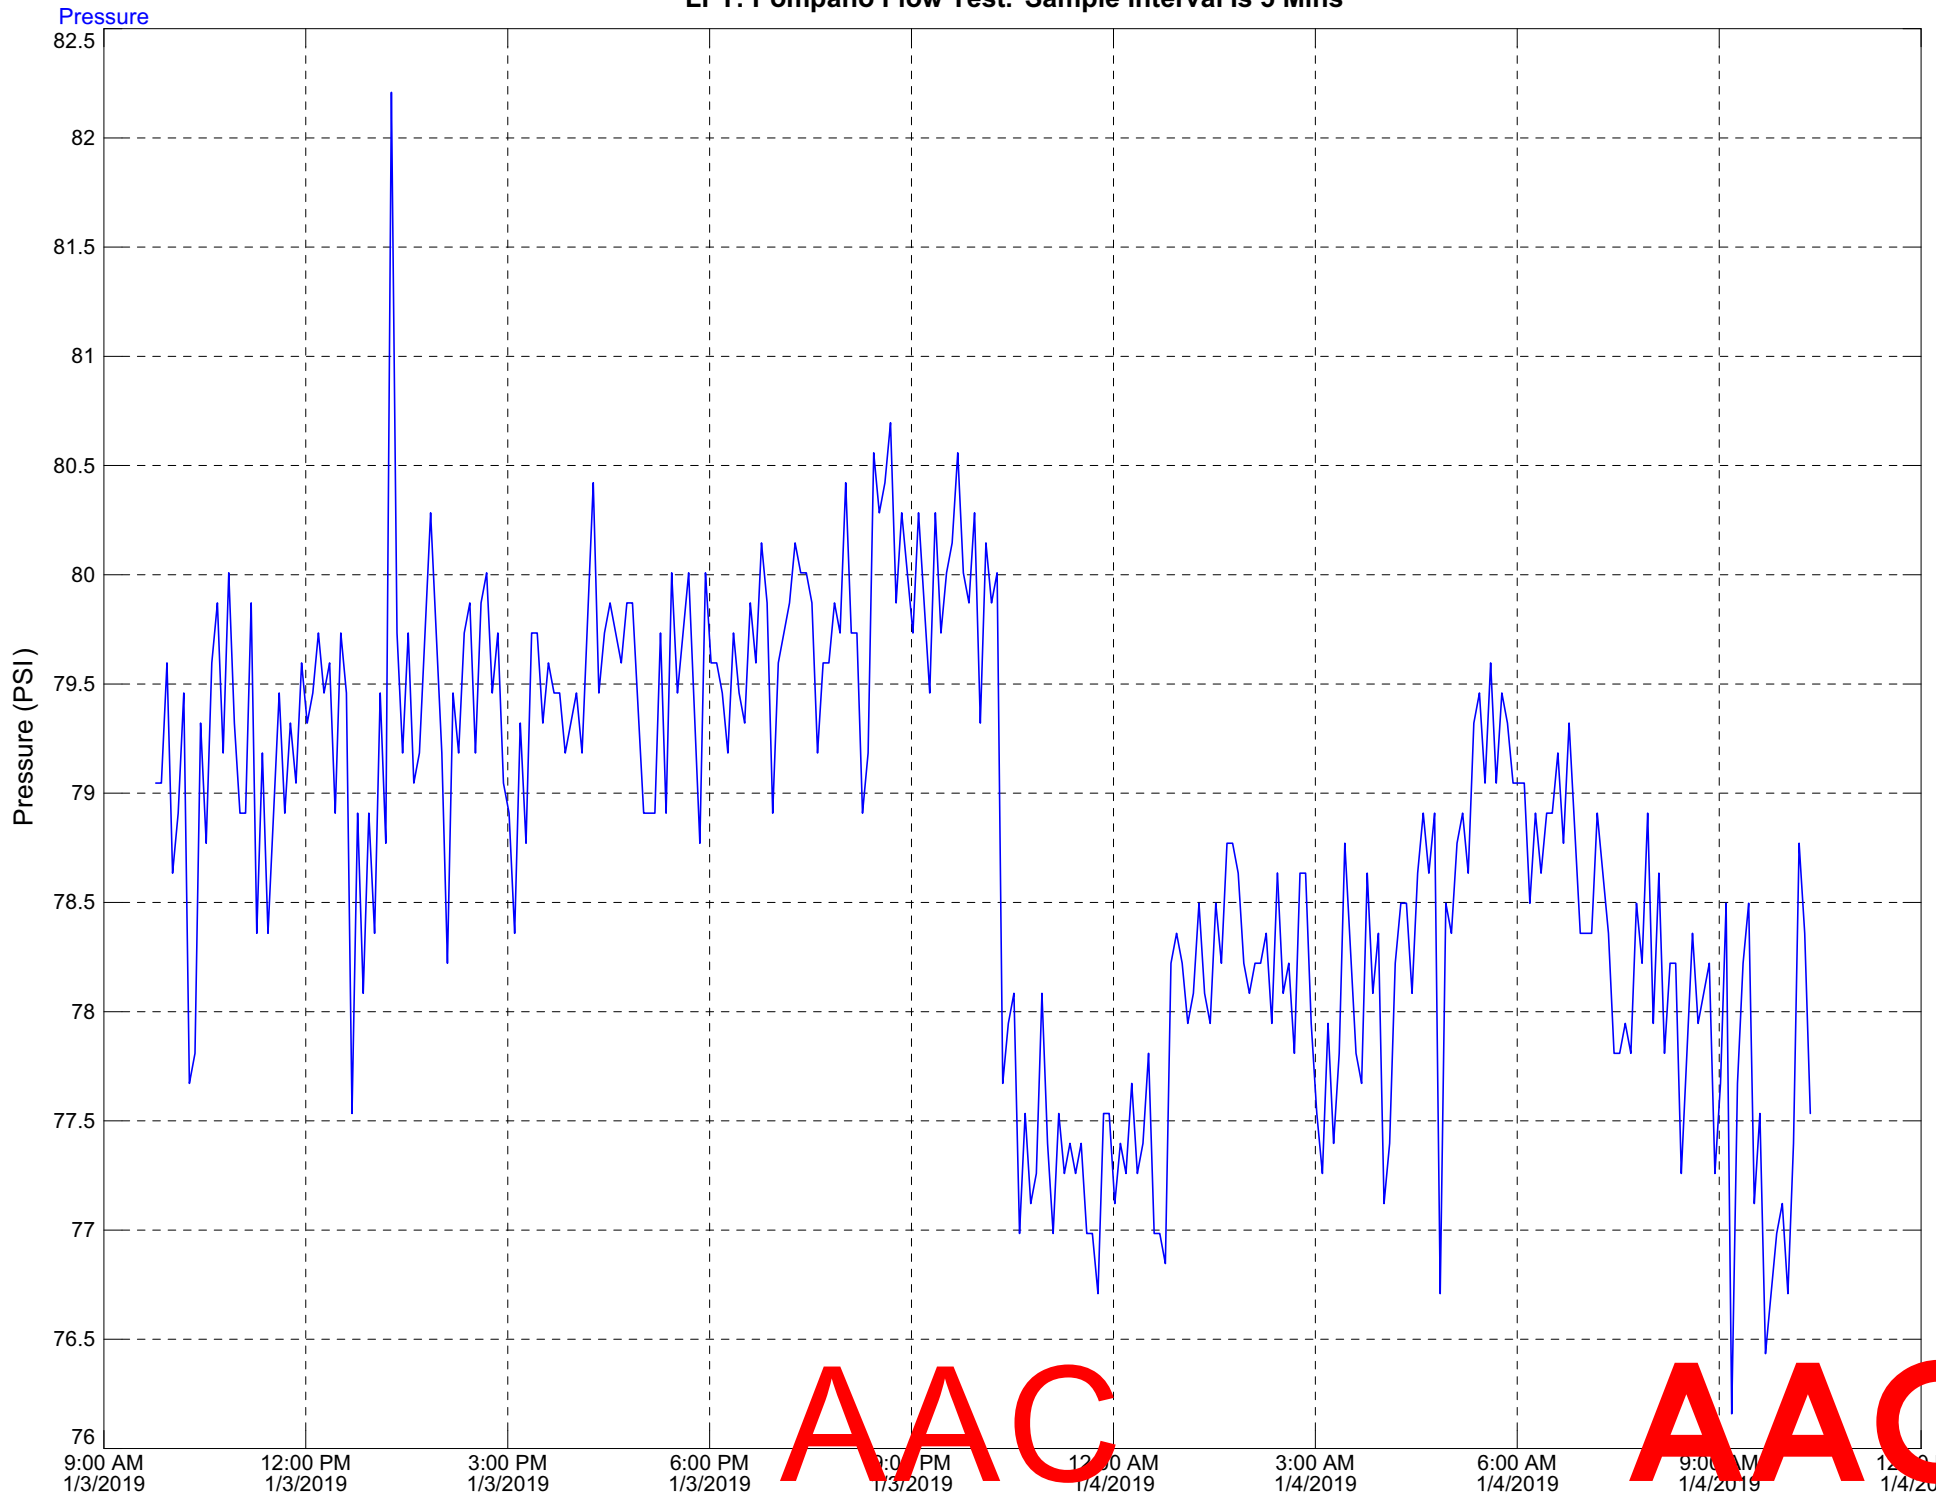

AAC

PZ18-1200030

07/06/2021

AAC

PZ18-1200030

04/02/2019